


Parameter	Value
1. α_1	0.0000
2. α_2	0.0000
3. α_3	0.0000
4. α_4	0.0000
5. α_5	0.0000
6. α_6	0.0000
7. α_7	0.0000
8. α_8	0.0000
9. α_9	0.0000
10. α_{10}	0.0000
11. α_{11}	0.0000
12. α_{12}	0.0000
13. α_{13}	0.0000
14. α_{14}	0.0000
15. α_{15}	0.0000
16. α_{16}	0.0000
17. α_{17}	0.0000
18. α_{18}	0.0000
19. α_{19}	0.0000
20. α_{20}	0.0000
21. α_{21}	0.0000
22. α_{22}	0.0000
23. α_{23}	0.0000
24. α_{24}	0.0000
25. α_{25}	0.0000
26. α_{26}	0.0000
27. α_{27}	0.0000
28. α_{28}	0.0000
29. α_{29}	0.0000
30. α_{30}	0.0000
31. α_{31}	0.0000
32. α_{32}	0.0000
33. α_{33}	0.0000
34. α_{34}	0.0000
35. α_{35}	0.0000
36. α_{36}	0.0000
37. α_{37}	0.0000
38. α_{38}	0.0000
39. α_{39}	0.0000
40. α_{40}	0.0000
41. α_{41}	0.0000
42. α_{42}	0.0000
43. α_{43}	0.0000
44. α_{44}	0.0000
45. α_{45}	0.0000
46. α_{46}	0.0000
47. α_{47}	0.0000
48. α_{48}	0.0000
49. α_{49}	0.0000
50. α_{50}	0.0000
51. α_{51}	0.0000
52. α_{52}	0.0000
53. α_{53}	0.0000
54. α_{54}	0.0000
55. α_{55}	0.0000
56. α_{56}	0.0000
57. α_{57}	0.0000
58. α_{58}	0.0000
59. α_{59}	0.0000
60. α_{60}	0.0000
61. α_{61}	0.0000
62. α_{62}	0.0000
63. α_{63}	0.0000
64. α_{64}	0.0000
65. α_{65}	0.0000
66. α_{66}	0.0000
67. α_{67}	0.0000
68. α_{68}	0.0000
69. α_{69}	0.0000
70. α_{70}	0.0000
71. α_{71}	0.0000
72. α_{72}	0.0000
73. α_{73}	0.0000
74. α_{74}	0.0000
75. α_{75}	0.0000
76. α_{76}	0.0000
77. α_{77}	0.0000
78. α_{78}	0.0000
79. α_{79}	0.0000
80. α_{80}	0.0000
81. α_{81}	0.0000
82. α_{82}	0.0000
83. α_{83}	0.0000
84. α_{84}	0.0000
85. α_{85}	0.0000
86. α_{86}	0.0000
87. α_{87}	0.0000
88. α_{88}	0.0000
89. α_{89}	0.0000
90. α_{90}	0.0000
91. α_{91}	0.0000
92. α_{92}	0.0000
93. α_{93}	0.0000
94. α_{94}	0.0000
95. α_{95}	0.0000
96. α_{96}	0.0000
97. α_{97}	0.0000
98. α_{98}	0.0000
99. α_{99}	0.0000
100. α_{100}	0.0000

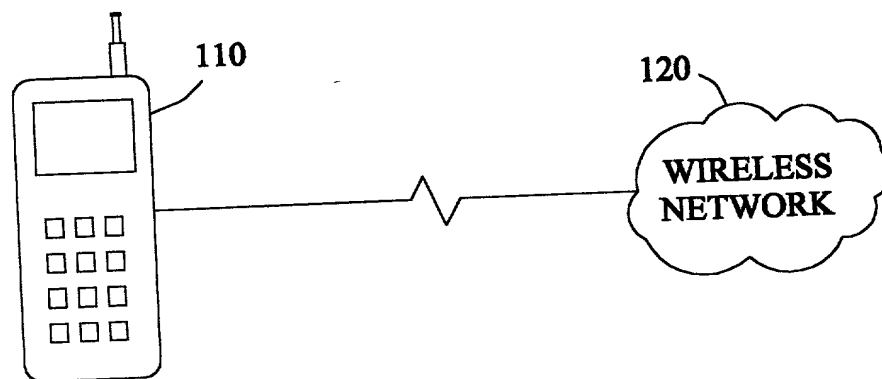

100  **FIG. 1**

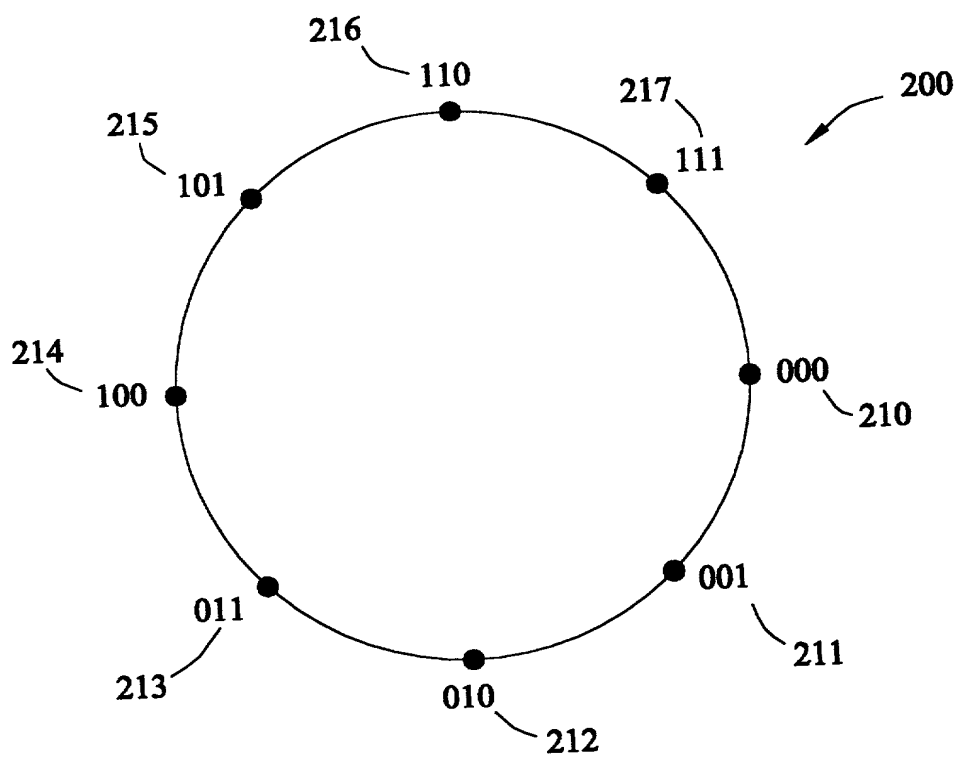


FIG. 2

300

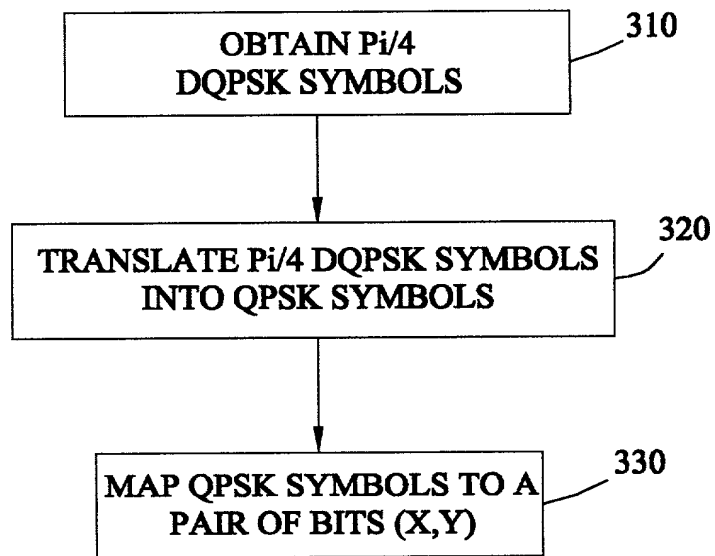


FIG. 3

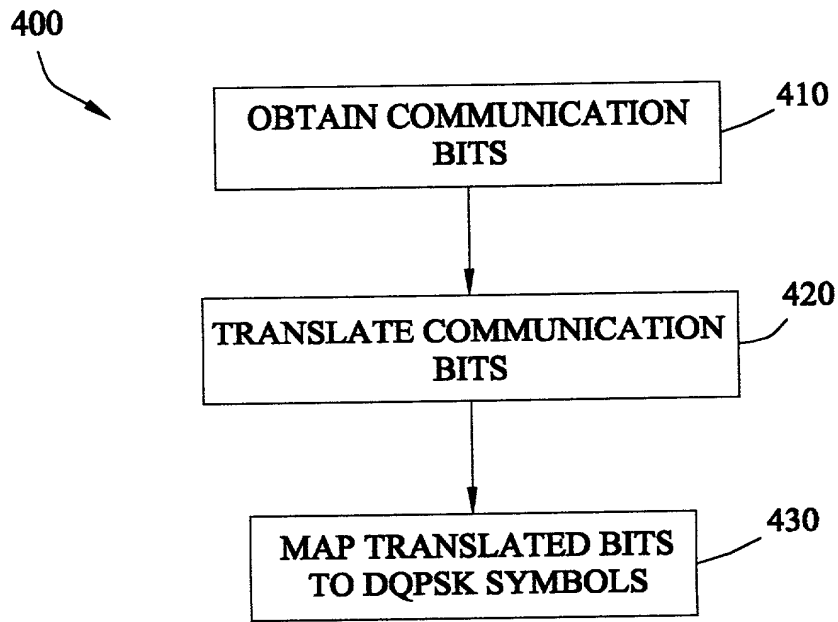


FIG. 4

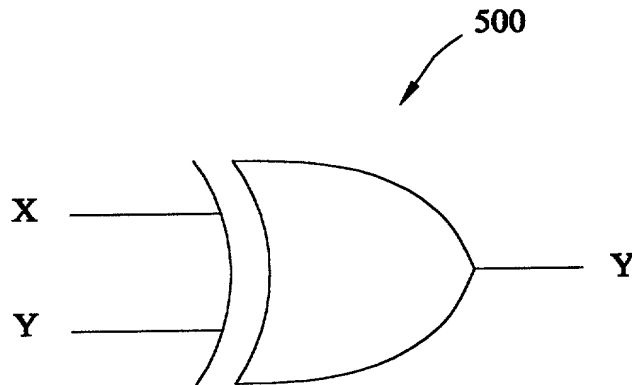


FIG. 5